



01

## EC - DECLARATION OF CONFORMITY

We,

Dwyer Instruments, Inc.  
P.O. Box 373  
Michigan City, IN 46361, USA  
(219) 879-8868

declare under our sole responsibility that our Series HM28, Handheld Digital Manometer, to which this declaration relates, are in conformity with the following EC Directives and harmonized standards:

Directive 2004/108/EC (EMC)

IEC 61326-1 (2012) Electrical Equipment for Measurement, Control, and Laboratory Use- EMC Requirements -Part I:  
General Requirements

IEC 61000-6-1: (2005) Electromagnetic compatibility (EMC) - Part 6-1: Generic standards - Immunity for Residential,  
Commercial and Light-Industrial Environments

IEC 61000-6-3 (2010) Electromagnetic compatibility (EMC) - Part 6-3: Generic Standards - Emission Standard for Residential,  
Commercial and Light-Industrial Environments


The authorized representative located within the Community is:

Dwyer Instruments Ltd  
Unit 16, The Wye Estate, London Road  
High Wycombe, Bucks HP11 1LH-U.K.  
(+44) (0) 1494 461707

On behalf of Dwyer Instruments, Inc.

Senior Regulatory Engineer

Michigan City, Indiana, USA  
6/20/14

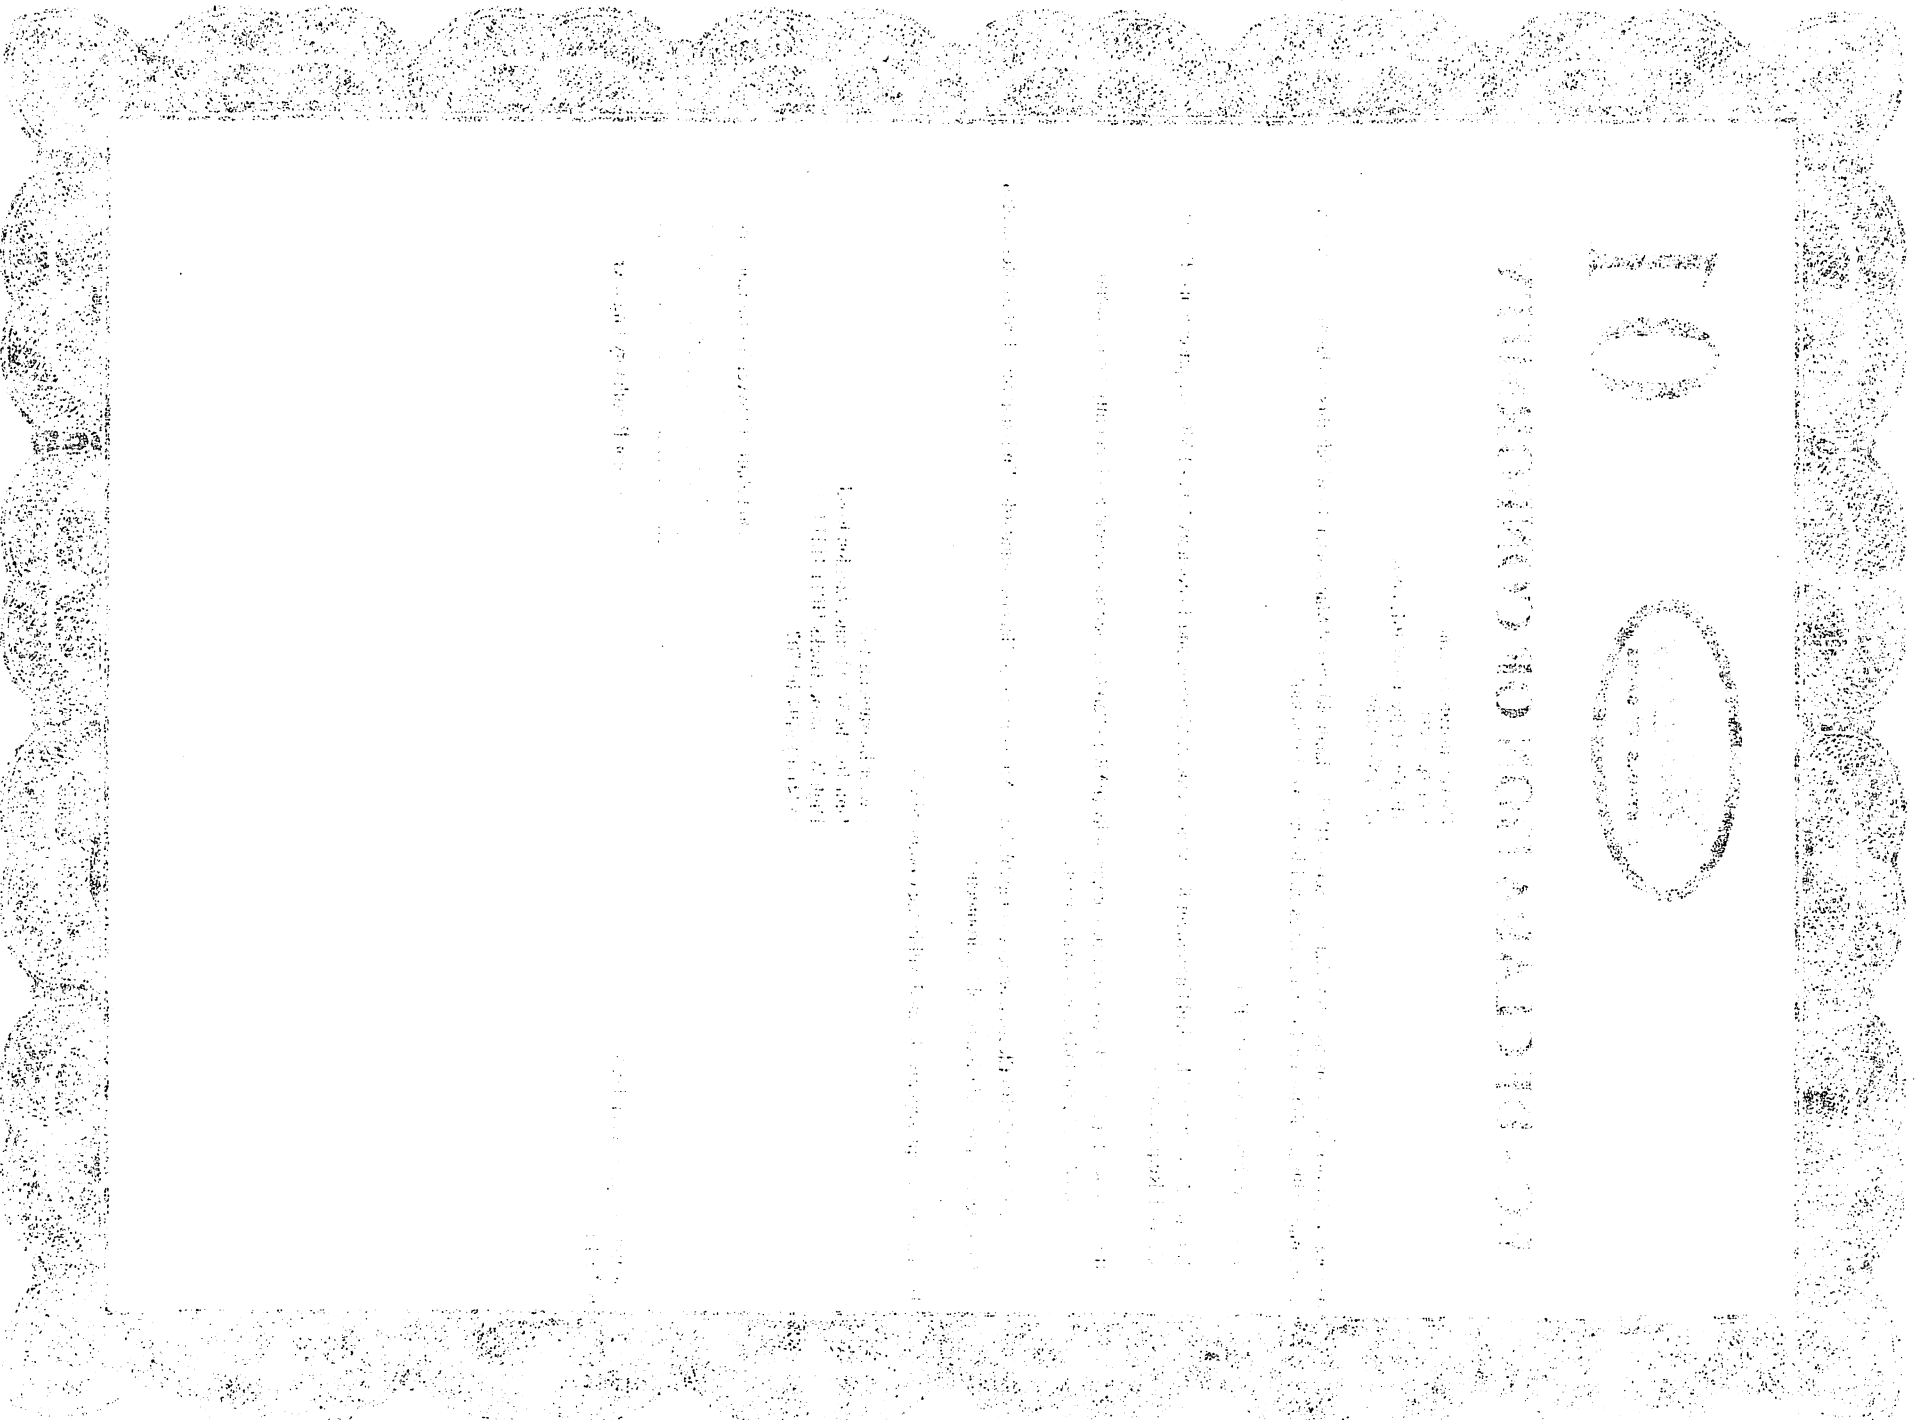

THE UNIVERSITY OF CALIFORNIA  
LIBRARY  
1925

THE UNIVERSITY OF CALIFORNIA  
LIBRARY  
1925

THE UNIVERSITY OF CALIFORNIA  
LIBRARY  
1925

THE UNIVERSITY OF CALIFORNIA  
LIBRARY  
1925

THE UNIVERSITY OF CALIFORNIA  
LIBRARY  
1925



1925